



Thrombodynamics Analyser

Thrombodynamics 4D assay



Patient:		01.01.2015 00:00
Age: , History N:		
Measurement title:	Example_dabigatran_2	kit PLS
Plasma type:	Fresh PFP	
Sample code:	Example_dabigatran_2	
Physician:		
Medical Institution/Department:		
Diagnosis:		
Prescribed medications:		



Fibrin dynamics parameters	Unit	Parameter	Value	Norm.
Rate of clot growth	um/min	V	39,9	
Lag time	min	Tlag	2,8	
Initial rate of clot growth	um/min	Vi	65,9	
Stationary rate of clot growth	um/min	Vst	39,9	
Clot size at 30 min	um	CS	1467	
Clot density	a.u.	D	48352	
Spontaneous clotting	min	Tsp		

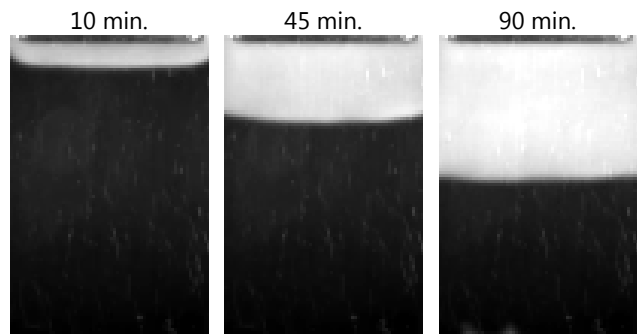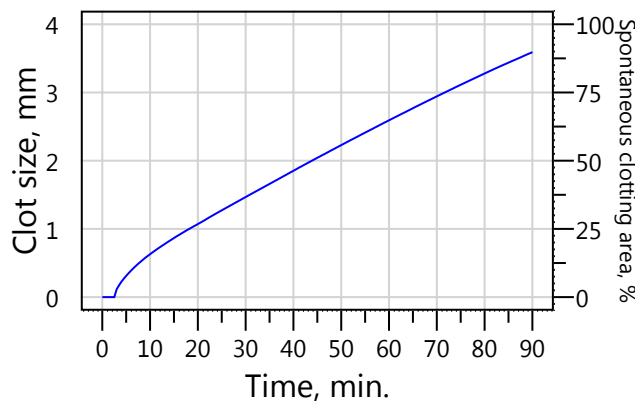

Thrombin dynamics parameters	Unit	Parameter	Value	Norm.
Stationary amplitude of thrombin peak	AU/L	Ast	29,0	
Rate of thrombin peak propagation	um/min	Vt	36,7	

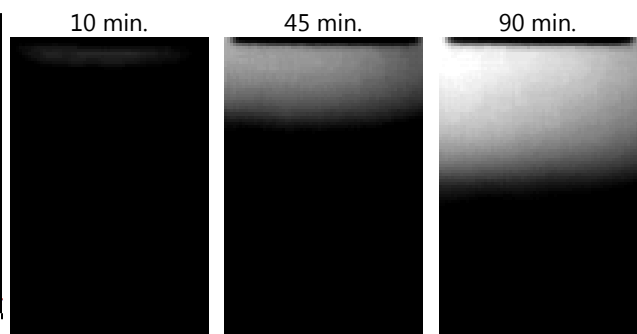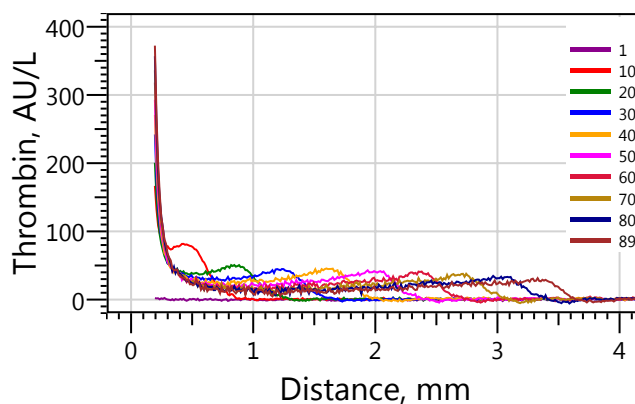

Tech info:
Comment:

ATTENTION: Research use only. The result are not be used for traetment pr diagnostic purposes.

Operator: , report created 07.07.2017 22:17


S/N: 210013

Thrombodynamics Analyser

Thrombodynamics 4D assay

Patient: Age: , History N:	01.01.2015 00:00
Measurement title: Example_dabigatran_2 Plasma type: Fresh PFP Sample code: Example_dabigatran_2 Physician: Medical Institution/Department: Diagnosis: Prescribed medications:	kit PLS

Activator thrombin generation (ATG) parameters	Unit	Parameter	Value	Norm.
Activator thrombin potential	AU*min/L	ETP_ATG	851,5	
ATG Maximum thrombin concentration	AU/L	Cmax_ATG	71,5	
ATG Lag time	min	Lag_ATG	2,2	
ATG Time to peak	min	Tmax_ATG	4,8	

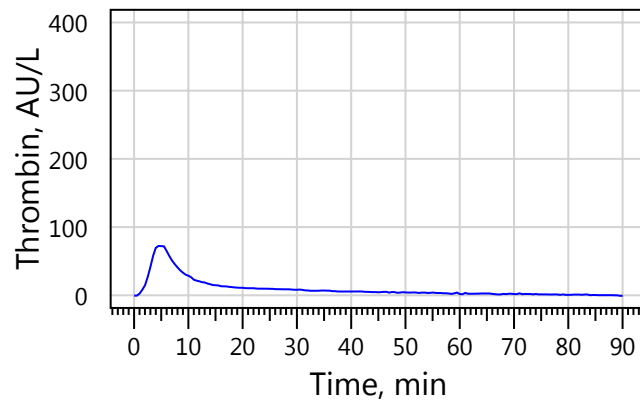

Tech info:
Comment:

ATTENTION: Research use only. The result are not be used for traetment pr diagnostic purposes.

Operator: , report created 07.07.2017 22:17

S/N: 210013



328995e0-da09-4558-9514-f5b3e437a2e0