

Thrombodynamics Analyser

Thrombodynamics assay



23.05.2018 13:43

Measurement title: Hypercoagulation+Hypofibrinogenemia TD
 Plasma type: Fresh PFP
 Sample code: Example TDX #6

TDX



Fibrin dynamics parameters	Unit	Parameter	Value	Norm.
Rate of clot growth	um/min	V	46,8	20,0-29,0
Lag time	min	Tlag	1,0	0,6-1,5
Initial rate of clot growth	um/min	Vi	72,4	38,0-56,0
Stationary rate of clot growth	um/min	Vst		20,0-29,0
Clot size at 30 min	um	CS		800-1200
Clot density	a.u.	D	9545	15000-32000
Spontaneous clotting	min	Tsp	22,9	30,0-

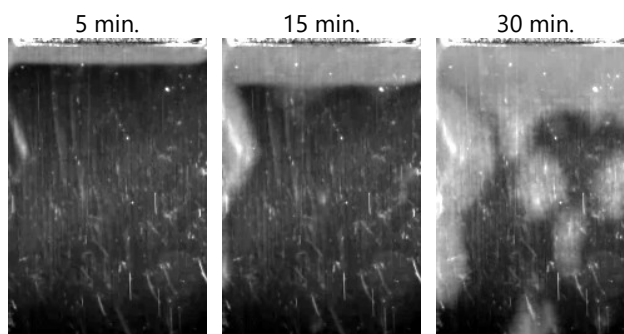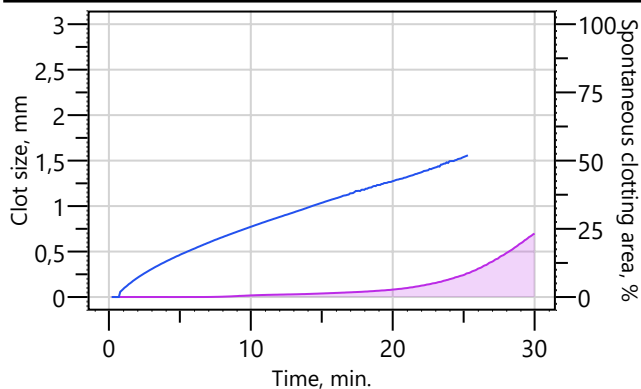

Comment:

Tech info:

ATTENTION: Research use only. Measurement results shouldn't be used for diagnostic purposes.

S/N: 000000, Operator: Operator, report created 29.03.2019 12:12